



Si device application

With *Nanofinder*[®] FLEX high resolution Raman imaging and precise Raman shift measurement are readily available.

High resolution Raman image with oil immersion objective lens (100x N.A. 1.4)

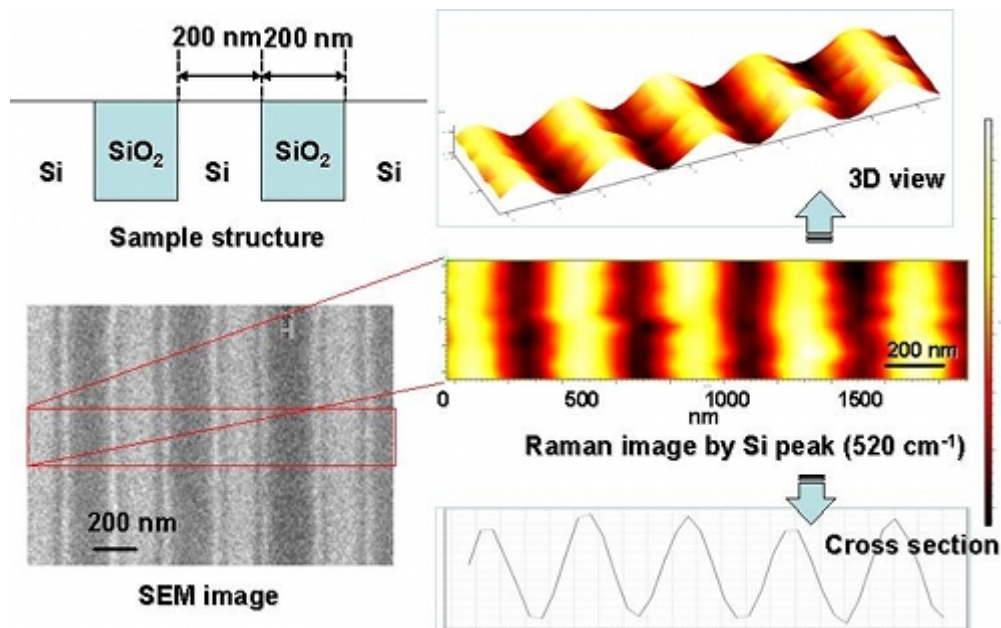

High resolution Raman image with air objective lens (100x N.A. 0.95)

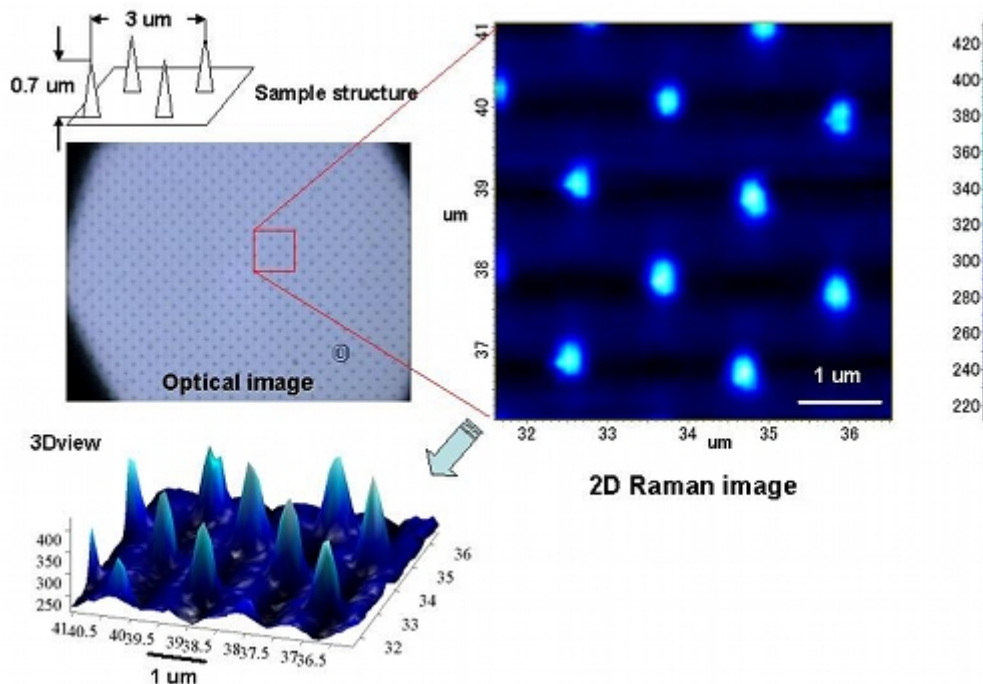

Fine Si Raman shift measurement

TII original "FitPeak" software was applied.

Sample structure

